

STIKO

Pressure
calibration
equipment



A pleasure to measure!





CONTENTS

Introduction	2
Oil operated deadweight testers	
DOS0015 (accuracy 0.015% of reading)	5
DOS0015 Dual Piston (accuracy 0.015% of reading)	6
DOS001 (accuracy 0.01% of reading)	7
DOS0008 (accuracy 0.008% of reading)	7
Gas driven, oil lubricated deadweight testers	
DGS001 (accuracy 0.01% of reading)	9
DGS0008 (accuracy 0.008% of reading)	10
DGDP001 Differential deadweight tester (accuracy 0.01% of reading)	10
Gas pressure regulators	
GPR120 S	11
GPR200 (for DGS001)	11
GPR200D (for DGDP001)	11
GPR200 SP	11
Comparison test pumps	
COP700/1400 (700/1400 bar)	12
MPC700	12
COP2500 (2500 bar)	13
COP4000/7000 (4000/7000 bar)	13
Accessories	
Dirt/moisture trap	14
Oxygen tester	14
Instrument stand	14
Adapters	14





INTRODUCTION

STIKO has more than 50 years experience in pressure equipment and calibrations and offers a complete line of pressure calibration equipment such as deadweight testers, comparison test pumps and a variety of accessories.

Deadweight testers

Deadweight testers are used as the basic primary standard and its principle is accepted all over the world for the most accurate pressure measurements.

No other piece of equipment for pressure measurement can match the stability, repeatability and accuracy of the deadweight tester. It is ideal for calibrating pressure transducers, pressure gauges, transfer standards, recorders, digital calibrators, etc. and can also be used to measure the pressure directly in systems and processes where precise measurements are important.

Basic principle of deadweight tester

A deadweight tester is based on a piston and cylinder assembly manufactured with extreme high accuracy. This cylinder is mounted in a column. The piston can rotate and freely move up and down. Accurately calibrated masses are loaded on top of the vertically mounted piston. A pressure is applied on the bottom of the piston to lift the piston with masses. This creates a balance between the downward force made by the masses and the upward force made by the pressure. With the known effective area of the Piston, the pressure can be calculated.


In formula:

$$p = \frac{F}{A}$$

p : pressure

F : force

A : area (of the piston)

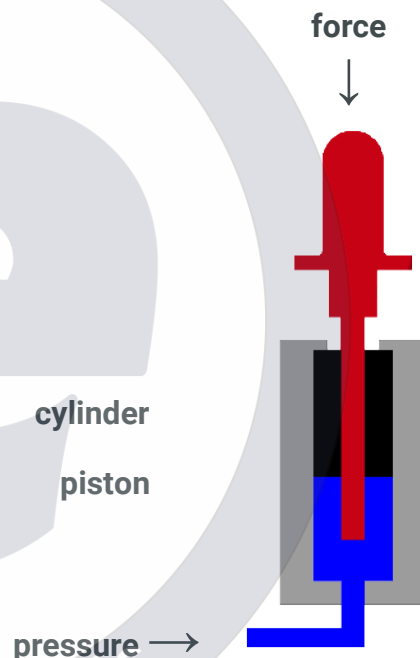

Piston cylinder assembly

The piston cylinder assembly is the heart of the deadweight tester and responsible for its high accuracy. STIKO manufactures piston cylinders with accuracies from 0.015% up to 0.008% of reading. To give an idea of the manufacturing skills, the space between the piston and the cylinder is in the μm range and can only be measured in a climatic room. To guarantee excellent Metro-logical characteristics, all pistons and cylinders are made of tungsten carbide. Because of the extreme hardness of this material, the pressure distortion (expansion) coefficient is negligible. The low friction coefficient provides minutes of turning with just a little swing of the masses.





Effective area

For all deadweight testers, the effective area is determined by cross floating with a known reference primary standard deadweight tester. The exact pressure can be calculated. In the below formula, compensation factors are listed for air buoyancy, local gravity, surface tension of the used oil and temperature and pressure expansion of the piston cylinder assembly.

$$p_e = \frac{m_c \cdot (1 - \rho_a / \rho_m) \cdot g_l + \tau \cdot \pi \cdot d}{A_{20,0} \cdot (1 + (\alpha_p + \alpha_c) \cdot (t - 20)) \cdot (1 + \lambda \cdot p_{nom})}$$


where:

p_e	: gauge pressure at reference level	[kPa]
m_c	: conventional mass	[kg]
$1 - \rho_a / \rho_m$: air buoyancy correction (= 0,99985)	[-]
g_l	: local gravity	[N/kg]
$\pi \cdot d$: piston circumference	[m]
τ	: surface tension oil (=0,031)	[N/m]
$A_{20,0}$: effective area at 20 °C / zero pressure	[m²]
$\alpha_p + \alpha_c$: thermal expansion coefficient piston + cylinder [°C-1]	
t	: piston cylinder temperature	[°C]
λ	: pressure distortion coefficient piston +cylinder [MPa-1]	
p_{nom}	: nominal working pressure	[MPa]

All necessary data are listed in the calibration certificate provided with each deadweight tester.

Mass set

The masses of the STIKO deadweight tester are made of non magnetic stainless steel. They are laser marked with a serial number and mass or the equivalent pressure. The weights are tared out to add stainless steel to an internal chamber. This is easy for recalibration or adjustments for gravity compensation. The mass of all weights are listed in the certificate. For small pressure steps, a box with small weights is optionally available.

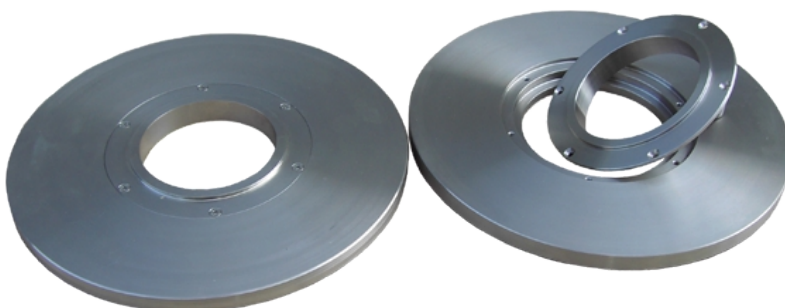



Pressure generating and control

The oil operated deadweight testers are supplied with a hand screw pump. This pump has a large displacement of 24cc, therefore a priming pump is not necessary. The pump is made of stainless steel as well as most other parts. The oil reservoir is combined with the vent valve and has a transparent cover to easily check the oil level. The vent valve has an easy to replace O-ring sealing. Because all used O-rings are listed in the manual, it is possible to buy them either at STIKO or at any other O-ring supplier.



Accuracy

STIKO manufactures deadweight testers with an accuracy from 0.015% up to 0.008% of reading. Without additional costs they can be calibrated according to the local gravity instead of the standard gravity of 9.80665 N/kg.

Certification

Deadweight testers with accuracy 0.015% of reading (model DOS0015) are delivered with a STIKO calibration certificate which is traceable to national and international standards. For the higher accuracies of 0.01 and 0.008% of reading, a third party *EA* certificate¹ is provided by Minerva Meettechniek B.V. Certification by any other national or international accredited laboratory is available at additional cost. We recommend a recalibration every 2 to 3 years depending on the amount of use.

Construction

All STIKO deadweight testers are of a simple well proven rugged construction. Most used material is stainless steel, and therefore a long life of the calibration standard is guaranteed.

Scope of delivery

All deadweight testers are delivered fully operational, with a stainless steel mass set in carrying cases.

The delivery includes:

- An English operating manual;
- A calibration certificate;
- $\frac{1}{8}$ ", $\frac{1}{4}$ ", $\frac{3}{8}$ ", $\frac{1}{2}$ " BSP female adapters;
- Spare multiseal for the pressure connection;
- A bottle of deadweight tester oil;
- A dust cover and bolts for mounting on a bench for type DOS001; DOS0008; DGS001, and DGDP001;



¹ European Accreditation, see <http://www.european-accreditation.org>



OIL DEADWEIGHT TESTERS

DOS0015

The oil operated deadweight tester DOS0015 has an accuracy of 0.015% of reading. This is a typical deadweight tester for industrial use and the weight set is transferred into a pressure unit. A traceable certificate is standard and a RVA certificate is possible as an option. The certificate shows the effective area as well as a list of the weight of each mass. The deadweight tester can be leveled with adjustable feet. An extra set of adjustable feet are included for fixing the deadweight tester to a bench. Five different pistons are available to cover ranges from 0.25 – 25 bar up to 10 – 1400 bar. Also ranges in psi, kPa, MPa and kg/cm² are available. The weight set can be adjusted according to the local gravity to eliminate errors. This is done free of charge.



Ranges

A list of masses corresponding with the ranges is listed below. For small pressure steps a fractional weight set is available as an option.

						Standard						Optional		
bar	Piston number and measuring range					mass set and equivalent of mass in bar								
mass set	No. 1		No. 2			0.25	0.025	0.05	0.25	0.5	2.5	5	0.0025	0.005
						0.5	0.05	0.1	0.5	1	5	10	0.005	0.01
	No. 3			1	0.1	0.2	1	2	10	20	0.01	0.02		
				No. 4		5	0.25	0.5	2.5	5	25	50	0.025	0.05
	No. 5	10	0.5			1	5	10	50	100	0.05	0.1		
kg	Range [bar]	Range [bar]	Range [bar]	Range [bar]	Range [bar]	carrier	number of masses							
20	0.25 - 25	0.5 - 50	1 - 100	5 - 250	10 - 500	1	1	4	1	4	1	4	1	4
24	0.25 - 30	0.5 - 60	1 - 120	5 - 300	10 - 600	1	1	4	1	4	1	5	1	4
28	0.25 - 35	0.5 - 70	1 - 140	5 - 350	10 - 700	1	1	4	1	4	1	6	1	4
32	0.25 - 40	0.5 - 80	1 - 160	5 - 400	10 - 800	1	1	4	1	4	1	7	1	4
36	0.25 - 45	0.5 - 90	1 - 180	5 - 450	10 - 900	1	1	4	1	4	1	8	1	4
40	0.25 - 50	0.5 - 100	1 - 200	5 - 500	10 - 1000	1	1	4	1	4	1	9	1	4
44	0.25 - 55	0.5 - 110	1 - 220	5 - 550	10 - 1100	1	1	4	1	4	1	10	1	4
48	0.25 - 60	0.5 - 120	1 - 240	5 - 600	10 - 1200	1	1	4	1	4	1	11	1	4
52	0.25 - 65	0.5 - 130	1 - 260	5 - 650	10 - 1300	1	1	4	1	4	1	12	1	4
56	0.25 - 70	0.5 - 140	1 - 280	5 - 700	10 - 1400	1	1	4	1	4	1	13	1	4

						Standard							Optional	
psi	Piston number and measuring range					Mass set and equivalent of mass in psi								
mass set	No. 1		No. 2			5	0,5	1	5	10	50	100	0.05	0.1
						10	1	2	10	20	100	200	0.1	0.2
	No. 3			20	2	4	20	40	200	400	0.2	0.4		
				No. 4		100	5	10	50	100	500	1000	0.5	1
	No. 5	200	10			20	100	200	1000	2000	1	2		
kg	Range [psi]	Range [psi]	Range [psi]	Range [psi]	Range [psi]	carrier	number of masses							
22	5 - 400	10 - 800	20 - 1600	100 - 4000	200 - 8000	1	1	4	1	4	1	3	1	4
28	5 - 500	10 - 1000	20 - 2000	100 - 5000	200 - 10000	1	1	4	1	4	1	4	1	4
33	5 - 600	10 - 1200	20 - 2400	100 - 6000	200 - 12000	1	1	4	1	4	1	5	1	4
39	5 - 700	10 - 1400	20 - 2800	100 - 7000	200 - 14000	1	1	4	1	4	1	6	1	4
44	5 - 800	10 - 1600	20 - 3200	100 - 8000	200 - 16000	1	1	4	1	4	1	7	1	4
50	5 - 900	10 - 1800	20 - 3600	100 - 9000	200 - 18000	1	1	4	1	4	1	8	1	4
55	5 - 1000	10 - 2000	20 - 4000	100 - 10000	200 - 20000	1	1	4	1	4	1	9	1	4



DOS0015 Dual Piston

The oil operated deadweight tester DOS0015 dual piston has the same features as the normal STIKO DOS0015. By using two pistons of different sizes, a larger measuring range is achieved. The pistons can easily be interchanged within minutes. A wooden box is used to safely store the pistons and cylinders.



Ranges

Both piston-cylinders assemblies could be used on one weight set. The piston-cylinders are made in such a way that the same weight creates for instance for the low range 10 bar and for the high range 100 bar.

For each combination of pistons, the table gives a list of masses corresponding with the ranges.

Piston number		No. 1	No. 2	No. 3	No. 4	No. 5
Ratio	1:	1	2	4	10	20

Example

If a deadweight tester is needed for 0.5 up to 1000 bar, a dual piston can be used.

See the table on page 5:

mass set of 40 kg (first column)

piston no. 2 gives 0.5 ... 100 bar

piston no. 5 gives 10 ... 1000 bar

Above table gives the piston ratio.

piston no. 2: ratio 2

piston no. 5: ratio 20

The ratio between both pistons is 2:20 or 1:10. The table on page 5 gives the weights needed to achieve above ranges. Piston no. 2 (0.5 ... 100 bar) is delivered with 9 weights of 10 bar. Using these same weights on piston no. 5 (10 ... 1000 bar) a pressure of 100 bar is made with each weight. Exactly 10 times more, ratio 1:10. With the same weight set on both pistons, an accuracy of 0.015% of reading is achieved.

Transport cases



Aluminum case



Flight case




DOS001

The oil operated deadweight tester DOS001 has an accuracy of 0.01% of reading. The weight column and pump are mounted on a stainless steel base plate. A triangle frame is used to make a steady and firm base for the weight column and can be leveled out by a spirit level. The weight carrier is of a hanging type and therefore insensible for any negative influences like friction of a support piston. The picture below shows the design of a DOS001. An EA RVA certificate by an accredited third party is standard. The certificate shows the effective area as well as the weight of each mass.



Design of DOS001/DOS0008

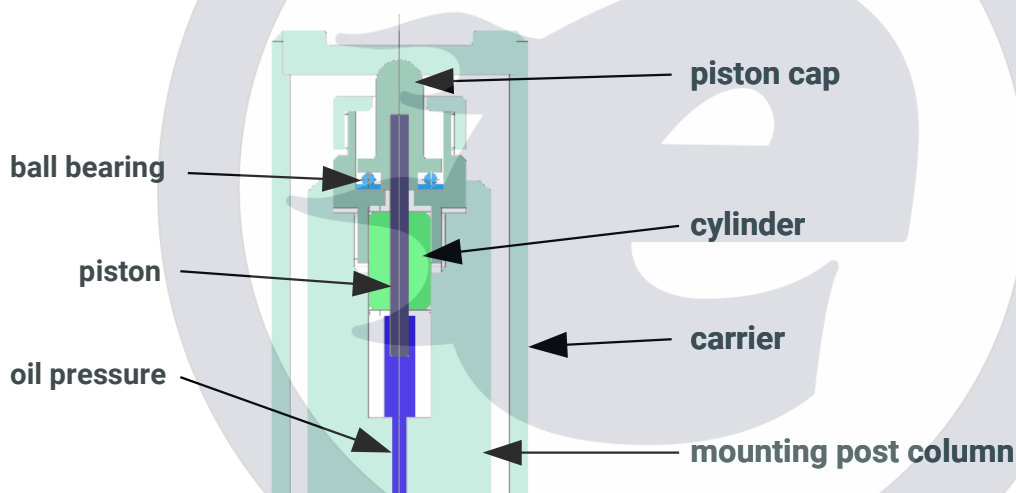

DOS0008

The oil operated deadweight tester DOS0008 has an accuracy of 0.008% of reading. The design is similar to the DOS001, but the piston cylinder assembly is even more accurate. To correct the temperature influence, a PT100 with LCD display is applied.





Mass set for DOS001 and DOS0008

The oil deadweight testers DOS001 and DOS0008 can be ordered with different mass sets: in kg, bar, psi or other pressure units. The best accuracy is achieved with the masses in kg and all known variables added in the mentioned formula. By ordering the mass set in a pressure unit, the deadweight tester can be used without using the formula. In this case the disagreement is larger than by using the formula, but still within 0.01% of reading for model DOS001 and 0.008% of reading for model DOS0008. The weight set can be adjusted to the local gravity to increase the accuracy and is done free of charge.

Ranges

A list of masses corresponding with the ranges is given below. Five different piston diameters are available to cover a wide pressure range. For small pressure steps, a fractional weights set is available as an option.

						Standard										Optional	
bar	Piston number and measuring range					Mass set and equivalent of mass in bar											
mass set	No. 1					1.25	0.025	0.05	0.125	0.25	0.5	1.25	2.5	5	10	0.0025	0.005
	No. 2					2.5	0.05	0.1	0.25	0.5	1	2.5	5	10	20	0.005	0.01
	No. 3					5	0.1	0.2	0.5	1	2	5	10	20	40	0.01	0.02
	No. 4					12.5	0.25	0.5	1.25	2.5	5	12.5	25	50	100	0.025	0.05
	No. 5					25	0.5	1	2.5	5	10	25	50	100	200	0.05	0.1
kg	Range bar	Range bar	Range bar	Range bar	Range bar	carrier	number of masses										
16	1.25-20	2.5-40	5-80	12.5-200	25-400	1	1	2	1	1	2	1	1	3	1	4	
24	1.25-30	2.5-60	5-120	12.5-300	25-600	1	1	2	1	1	2	1	1	5	1	4	
32	1.25-40	2.5-80	5-160	12.5-400	25-800	1	1	2	1	1	2	1	1	7	1	4	
40	1.25-50	2.5-100	5-200	12.5-500	25-1000	1	1	2	1	1	2	1	1	9	1	4	
48	1.25-60	2.5-120	5-240	12.5-600	25-1200	1	1	2	1	1	2	1	1	11	1	4	
56	1.25-70	2.5-140	5-280	12.5-700	25-1400	1	1	2	1	1	2	1	1	13	1	4	
64*					40-1600	1	1	2	1	1	2	1	1	15	1	4	
80*					40-2000	1	1	2	1	1	2	1	1	19	1	4	
100*					40-2500	1	1	2	1	1	2	1	1	24	1	4	

* DOS001 high: modified design see picture on page 16

						Standard										Optional		
psi	Piston number and measuring range					Mass set and equivalent of mass in psi												
mass set	No. 1					20	0.5	1	2.5	5	10	25	50	100	0.05	0.1		
			No. 2			40	1	2	5	10	20	50	100	200	0.1	0.2		
			No. 3			80	2	4	10	20	40	100	200	400	0.2	0.4		
			No. 4			200	5	10	25	50	100	250	500	1000	0.5	1		
			No. 5			400	10	20	50	100	200	500	1000	2000	1	2		
kg	Range psi	Range psi	Range psi	Range psi	Range psi	carrier	number of masses											
16	20-300	40-600	100-1200	200-3000	400-6000	1	1	2	1	1	2	1	1	2	1	4		
22	20-400	40-800	100-1600	200-4000	400-8000	1	1	2	1	1	2	1	1	3	1	4		
28	20-500	40-1000	100-2000	200-5000	400-10000	1	1	2	1	1	2	1	1	4	1	4		
33	20-600	40-1200	100-2400	200-6000	400-12000	1	1	2	1	1	2	1	1	5	1	4		
39	20-700	40-1400	100-2800	200-7000	400-14000	1	1	2	1	1	2	1	1	6	1	4		
44	20-800	40-1600	100-3200	200-8000	400-16000	1	1	2	1	1	2	1	1	7	1	4		
50	20-900	40-1800	100-3600	200-9000	400-18000	1	1	2	1	1	2	1	1	8	1	4		
55	20-1000	40-2000	100-4000	200-10000	400-20000	1	1	2	1	1	2	1	1	9	1	4		
80*					500-30000	1	1	2	1	1	2	1	1	14	1	4		
100*					500-36000	1	1	2	1	1	2	1	1	17	1	4		


* DOS001 high: modified design see picture on page 16



GAS DRIVEN, OIL LUBRICATED DEADWEIGHT TESTERS

DGS001

The gas operated deadweight tester DGS001 has an accuracy of 0.01% of reading. The piston cylinder assembly is made of tungsten carbide which is extremely hard and wear-resistant. The weight column is mounted on a stainless steel base plate. A triangle frame is used to make a steady and firm base for the weight column and can be leveled out by a spirit level. The weight carrier is of a hanging type and therefore insensible for any negative influences like friction of a support piston. An *EA* RVA certificate by an accredited third party is standard. The certificate shows the effective area as well as the weight of each mass.

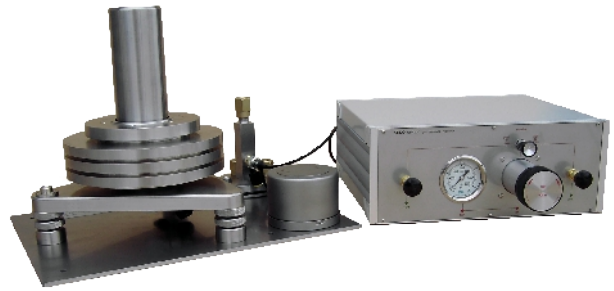


Oil lubricated / gas operated

The STIKO oil lubricated / gas operated piston of the DGS series is specially designed to have superior performance at higher gas pressures without the problems of gas lubricated / gas operated pistons cylinders. They have better sensitivity than oil lubricated pistons, however the natural drop rate is much higher at high line-pressure. This makes them very difficult to operate. Oil lubricated pistons have no significant drop rate as the oil acts as a seal.

There are a lot of deadweight tester manufacturers who claim oil lubrication / gas operation, but they use a traditional oil / oil piston and an oil-gas interface. The biggest and obvious disadvantage of this solution is that the surface level of the oil-gas interface has to be known precisely. The added uncertainty, especially in high line-pressure applications, make this solution not ideal. The piston cylinder assembly of the DGS series is significantly different. The oil is lead to the gap between piston and cylinder by means of an oil reservoir around the cylinder. As the oil surface is slightly higher than the entry bore in the cylinder, the oil pressure is also slightly higher than the gas pressure, ensuring enough lubrication between piston and cylinder. The benefits of this design are:

- excellent turning time of the piston;
- very small fall rate (also at higher pressures);
- excellent leak rate, because the oil acts as a seal;
- the oil avoids dirt and dust entrance between piston and cylinder.

Design of DGS001

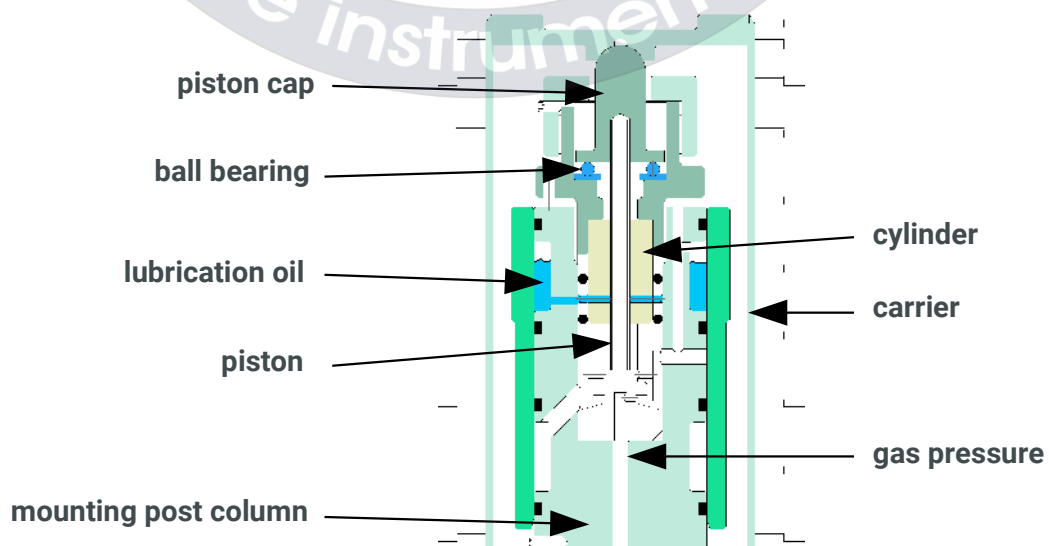



Ranges

A list of masses corresponding with the ranges is listed below. Three different piston cylinder assemblies are available. For small pressure steps, a fractional weight set is optionally available.

				Standard										Optional	
bar	Piston number and measuring range			Mass set and equivalent of mass in bar											
mass set	No. 1			1.25	0.025	0.05	0.125	0.25	0.5	1.25	2.5	5	0.0025	0.005	
		No. 2		2.50	0.05	0.1	0.25	0.5	1	3	5	10	0.005	0.01	
			No. 3	5	0.1	0.2	0.5	1	2	5	10	20	0.01	0.02	
kg	Range [bar]	Range [bar]	Range [bar]	carrier	number of masses										
16	1.25 - 20	2.5 - 40	5 - 80	1	1	2	1	1	2	1	1	3	1	4	
24	1.25 - 30	2.5 - 60	5 - 120	1	1	2	1	1	2	1	1	5	1	4	
32	1.25 - 40	2.5 - 80	5 - 160	1	1	2	1	1	2	1	1	7	1	4	
40	1.25 - 50	2.5 - 100	5 - 200	1	1	2	1	1	2	1	1	9	1	4	
48	1.25 - 60	2.5 - 120	-	1	1	2	1	1	2	1	1	11	1	4	
56	1.25 - 70	2.5 - 140	-	1	1	2	1	1	2	1	1	13	1	4	


				Standard									Optional	
psi	Piston number and measuring range			Mass set and equivalent of mass in psi										
mass set	No. 1			20	0,5	1	2.5	5	10	25	50	100	0.05	0.1
		No. 2		40	1	2	5	10	20	50	100	200	0.1	0.2
			No. 3	80	2	4	10	20	40	100	200	400	0.2	0.4
kg	Range [psi]	Range [psi]	Range [psi]	carrier	number of masses									
16	20 - 300	40 - 600	100 - 1200	1	1	2	1	1	2	1	1	2	1	4
22	20 - 400	40 - 800	100 - 1600	1	1	2	1	1	2	1	1	3	1	4
28	20 - 500	40 - 1000	100 - 2000	1	1	2	1	1	2	1	1	4	1	4
33	20 - 600	40 - 1200	100 - 2400	1	1	2	1	1	2	1	1	5	1	4
39	20 - 700	40 - 1400	100 - 2800	1	1	2	1	1	2	1	1	6	1	4
44	20 - 800	40 - 1600	-	1	1	2	1	1	2	1	1	7	1	4

DGS0008

The gas operated deadweight tester DGS0008 has an accuracy of 0.008% of reading. The design is similar to the DGS001, but the piston cylinder assembly is even more accurate. To correct the temperature error a PT100 with LCD display is installed.

DGDP001, Differential deadweight tester

The gas operated deadweight tester is also available in a differential pressure model. The DGDP001 combines the benefits of the oil lubricated piston cylinder assembly with the need to calibrate at a specific static pressure. This deadweight tester allows you to make differential pressure from 1.25 mbar up to the maximum pressure of 200 bar with static pressures from 5 bar up to 200 bar. As the accuracy of the DGDP is 0.01% of reading, it can be used to calibrate differential pressure transmitters of 0.1 or 0.05%. A differential regulator (model GPR200D, page 11) is used to set the line (static) pressure and to add the differential pressures.

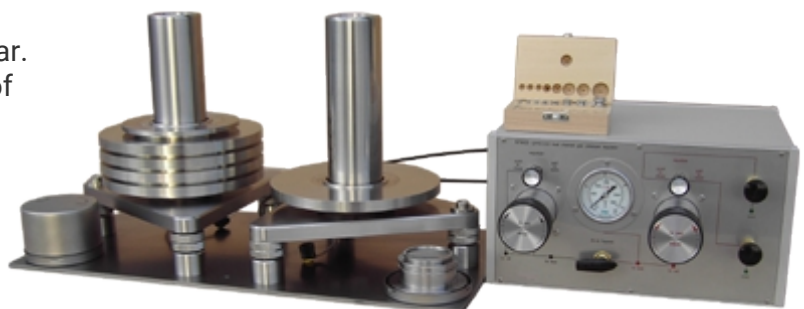



GAS PRESSURE REGULATORS

Gas pressure regulators are used to regulate and fine tune gas pressures. They are necessary in combination with gas deadweight testers, but can also be used for other calibration purposes such as a calibration setup with a digital reference instrument. All regulators must be connected to a bottle of compressed nitrogen or any other gas. The maximum inlet pressure is 200 bar. All regulators are equipped with Minimesse flexible tubing.

GPR120 S

This gas pressure regulator is an easy to use max. 120 bars regulator with a fine to adjust inlet and vent valve. The reference and instrument under test can be mounted directly on top of the housing. Adapters with $\frac{1}{8}$ ", $\frac{1}{4}$ ", $\frac{3}{8}$ ", $\frac{1}{2}$ " BSP female thread are included as well as Minimesse tubing to connect it to a nitrogen filled bottle.



GPR200

This gas pressure regulator is a regulator with an extreme fine to adjust variable volume. It is especially designed to work with the gas driven deadweight tester DGS001. Minimesse tubing is included to connect it to a nitrogen filled bottle.



GPR200 D

This gas pressure regulator is a double GPR200 regulator. It is specially designed to combine with the gas driven differential deadweight tester DGDP001 (page 10). A by-pass valve is used to isolate the high and low regulators. Minimesse tubing is included to connect it to a nitrogen filled bottle.



GPR200 SP

This gas pressure regulator is a GPR200 with built-in pressure reducer. By reducing the pressure just above the required pressure, an even better pressure adjustment can be achieved. Minimesse connections are located at the back as well on the front of the housing.





COMPARISON TEST PUMPS


Comparison test pumps are used for checking pressure instruments against a master test gauge or transducers. They are portable and rugged. A stainless steel bottom plate with mounting holes is used for stable bench mounting.

COP700/1400

This large volume (26cc) comparison test pump is easy to operate. The oil reservoir is combined with the vent valve and has a transparent cover to easily check the oil level. The vent valve has an easy to replace O-ring sealing. Because all used O-rings are listed in the manual, it is possible to buy them either at STIKO or at a local parts store. All pumps are delivered with adapters to $\frac{1}{8}$ ", $\frac{1}{4}$ ", $\frac{3}{8}$ ", $\frac{1}{2}$ " BSP female thread. Aluminum cases or flight cases are available for transport: see page 6.

A variety of models are available:

Model	Medium	Pressure bar	Option
COP700	oil	0 - 700	Skydrol
COP1400	oil	0 - 1400	-
COP700 water	water	0 - 700	cleaned for oxygen use
COP1000 water	water	0 - 1000	cleaned for oxygen use

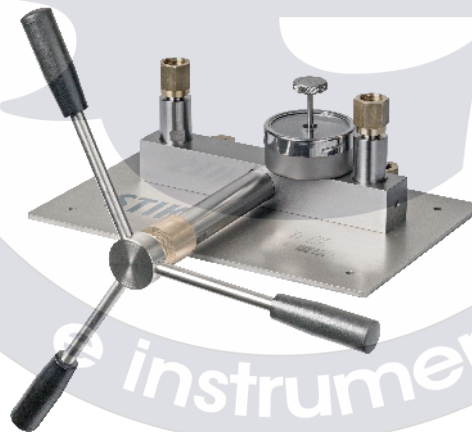

MPC700

The Micro Pressure Controller is designed for setting the pressure of the comparison test pump COP700 in a more accurate way than the standard version. No modifications to the original COP-system are necessary to mount the MPC-700. Also available as an after sales kit.





COP2500

This high pressure comparison test pump works up to 2500 bar. All components are mounted in a strong rugged stainless steel frame. A polycarbonate transparent cover protects the operator at all times. A priming pump is used to purge the system and after priming, a hand pump is used to set accurately the required pressure. The priming pump, valve and high pressure hand pump can be operated from the front. The pressure connections are of 9/16" UNF high pressure type.



***A pleasure
to measure!***

COP4000 / COP7000

This ultra high pressure comparison test pump makes a maximum pressure of 4000 bar for COP4000 and 7000 bar for the COP7000 model. All components are mounted in a strong rugged stainless steel frame to protect the operator at all times. All handles and valves can be operated from the front. Therefore the operator is always safe.

A priming pump of 26cc is applied to prime the system and to operate up to 700 bar. The large high pressure hand pump is used to obtain the maximum pressure. A large oil reservoir of 0.7 liter with transparent cover is applied to check the oil level. All ports can be shut off by high pressure valves to isolate a specific circuit.




Optional with highly accurate transducer (4000 bar or 7000 bar) and display.



ACCESSORIES

Dirt / moisture trap (max. 200 bar)

This stainless steel dirt / moisture trap is used to protect pneumatic calibration systems from dirt and oil. Any dirt and moisture can be seen through the inspection glass. The maximum allowable pressure is 200 bar. It is delivered with a free standing frame and a $\frac{1}{8}$ ", $\frac{1}{4}$ ", $\frac{3}{8}$ ", $\frac{1}{2}$ " BSP female adapter set. The unit can be supplied with a filter unit which is easy to drain by means of a drain plug.

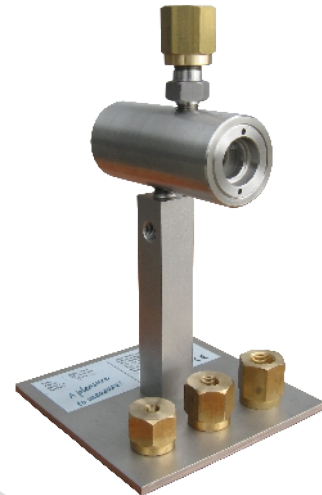

Oxygen tester (max. 700 bar)

Oxygen devices have to be absolutely free from oil and grease. Also, many other devices have to be kept clean. They have to be tested on air, water or other suitable liquids. This oxytester (oil-water separator) guarantees an absolute separation between the liquid of the reference calibration equipment and the liquid of the device under test. The separator is sometimes used to prevent a tester from being contaminated by solids or liquids from gauges being calibrated. It is delivered with a free standing frame and a $\frac{1}{8}$ ", $\frac{1}{4}$ ", $\frac{3}{8}$ ", $\frac{1}{2}$ " BSP female adapter set.

Instrument stand

This stainless steel instrument stand is used to connect pressure gauges, transducers and other pressure equipment. The instrument stand is supplied with a $\frac{1}{8}$ ", $\frac{1}{4}$ ", $\frac{3}{8}$ ", $\frac{1}{2}$ " BSP female adapter set and a minimess quick tubing connection. The maximum pressure is limited by the minimess tubing. With stainless steel capillary or high pressure tube, higher pressures can be achieved.




Adapters

A large variety of adapters can be supplied like angle adapters and adapters with a special thread i.e. autoclave or other high pressure connections. For instruments under test with NPT thread a $\frac{1}{8}$ ", $\frac{1}{4}$ ", $\frac{3}{8}$ ", $\frac{1}{2}$ " NPT female and for metric thread: M10, M12, M14, M20 adapter sets are available in brass. Adapters in stainless steel can also be supplied.



STIKO

Pressure
calibration
equipment

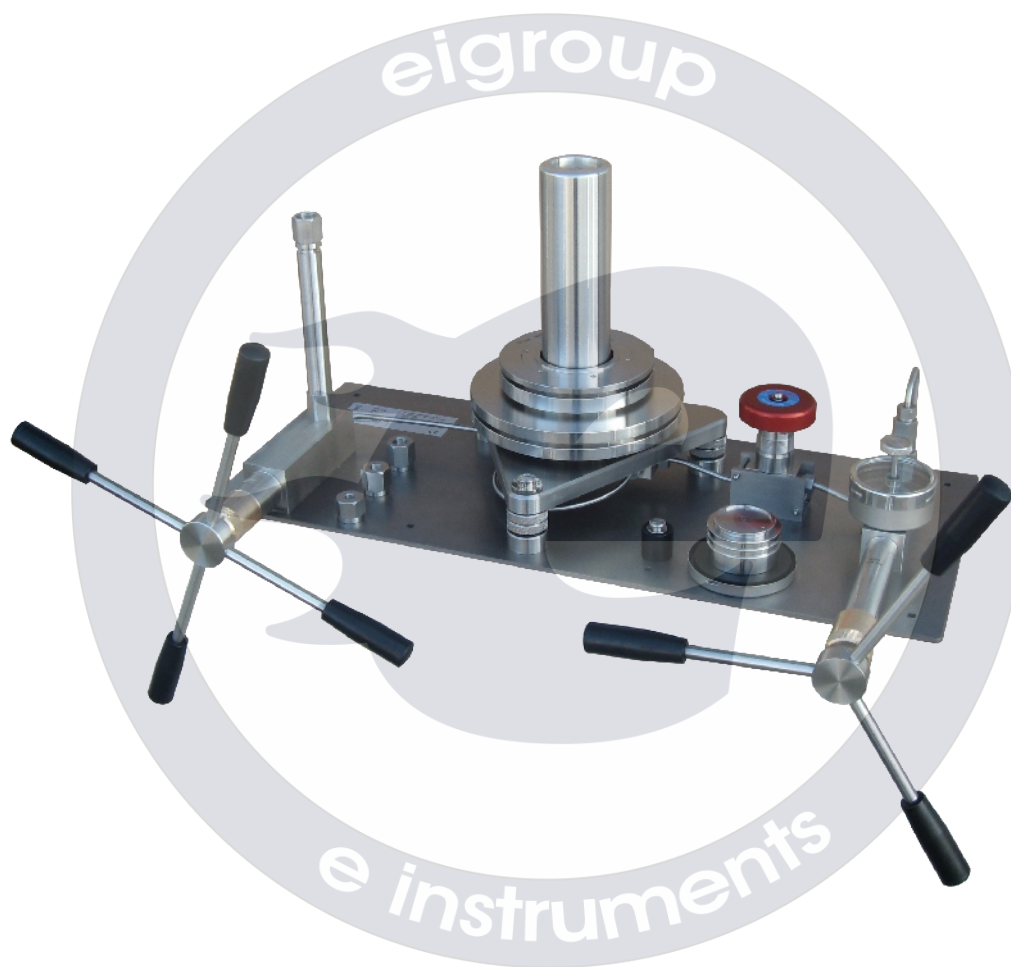

***A pleasure
to measure!***